Ozcanium Analytics
ABN: 14 754 514 569
Ozcaniumanalytics.com.au
+61 407 260 481


Certificate of Analysis

KLOW 80mg

Compound	: KLOW	**Net Content**	: GHK-CU: 49.28mg
Lot Number	: 08/09/2026		KPV: 9.45mg
Analysis date	: 12/09/2026		BPC-157: 9.53mg
Method	: UPLC-MS/MS		TB-500: 9.29mg
Verification	: OZ-HPLCMS-XCG1	**Client**	: Coregenyx Pty Ltd
Purity	: 98.93%		Coregenyx.com



Ultra Performance Liquid Chromatography (UPLC-UV) Chromatogram

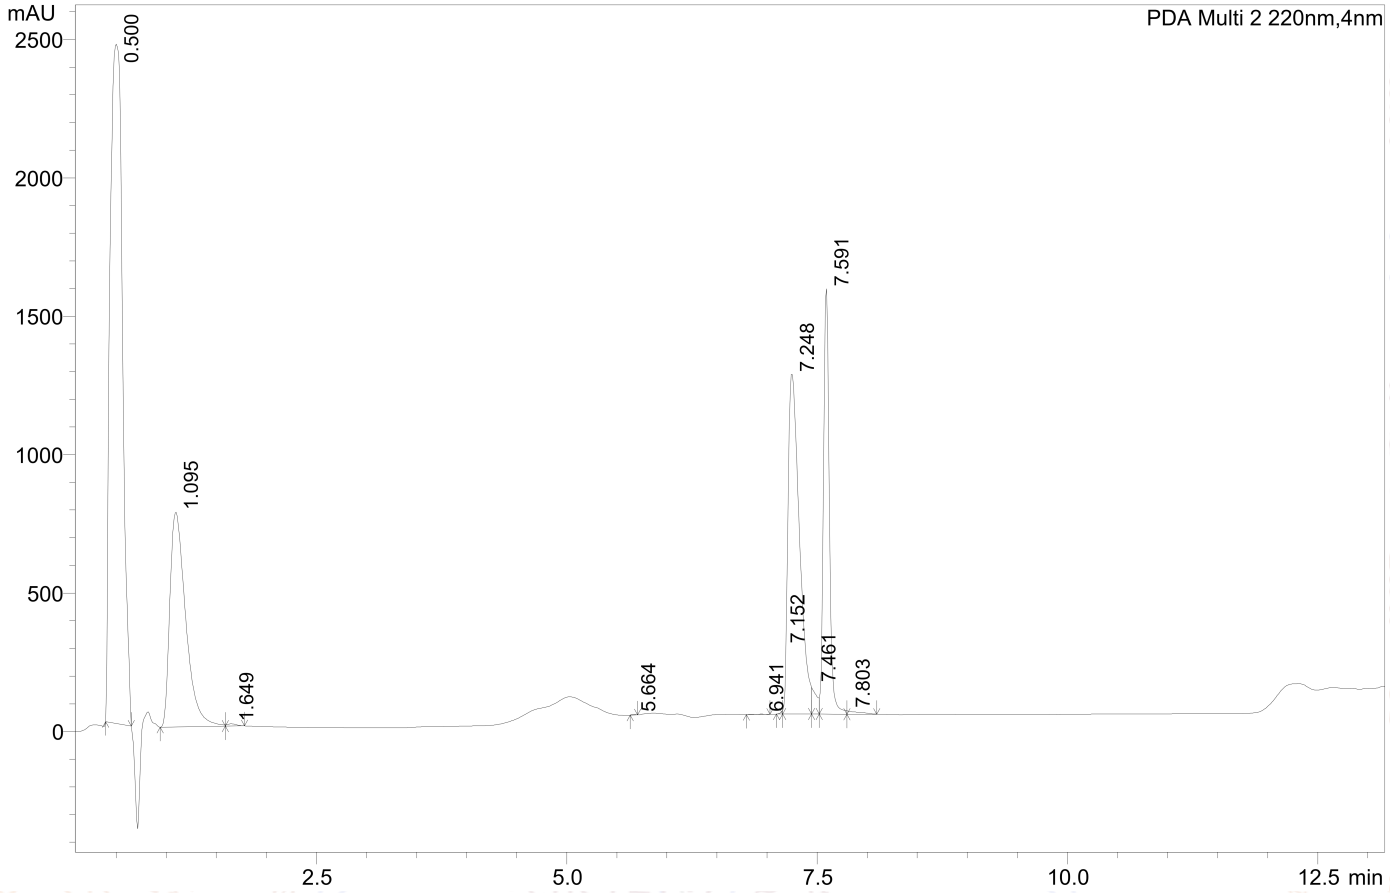

PEAK LIST

Peaks Detected: 10

#	Time (min)	Area	%Area	Assignments
1	0.500	21334420	45.943	GHK-CU
2	1.095	8563466	18.441	KPV
3	1.649	52588	0.113	
4	5.664	7821	0.017	
5	6.941	10558	0.023	
6	7.152	20775	0.045	
7	7.248	9830544	21.170	BPC-157
8	7.461	316706	0.682	
9	7.591	6209735	13.373	TB-500
10	7.803	89728	0.193	

Analysis by Ibrahim A. Ozcan,
Lead Chemist Ozcanium Analytics
Signature



Report Compiled by Zein S. Sabini
14/09/2026

Note: Sample may contain salts and sugars, as standard additives. These are not considered impurities and are not included in the peak list

© Copyright 2026 by Ozcanium Analytics. All rights reserved.

Ozcanium Analytics
ABN: 14 754 514 569
Ozcaniumanalytics.com.au
+61 407 260 481

GHK-CU

CAS Number : 49557-75-7

PubChem CID : 133697840

Liquid Chromatography Mass Spectrometry (LC-MS) Identity Analysis

Identity confirmation with SIM


Analysis date : 12/09/2026

Monitored Ion Channels (SIM):

Monitored (m/z):	Detected (m/z):
363	363.35
403	402.60
805	805.15

Detection Assignment: GHK-CU

Collected Mass Spectrum

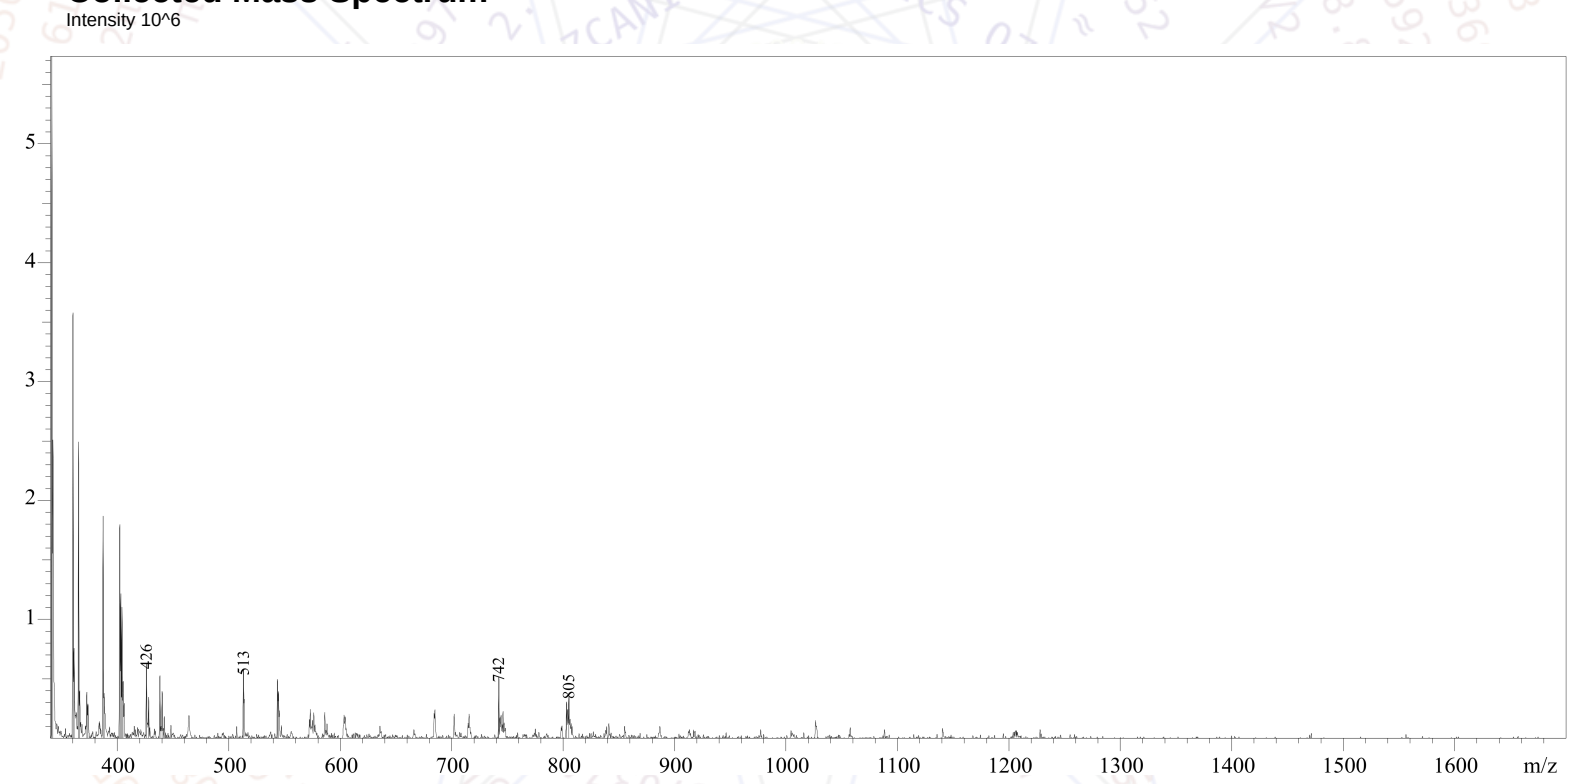

Note : Monoisotopic m/z values are not easily seen in full spectrum view for larger molecules and peptides.

The recorded fragmentation pattern may differ between systems, and vary based on method.

Analysis by Ibrahim A. Ozcan,
Lead Chemist Ozcanium Analytics
Signature

Report Compiled by Zein S. Sabini
14/09/2026

© Copyright 2026 by Ozcanium Analytics. All rights reserved.

Ozcanium Analytics
ABN: 14 754 514 569
Ozcaniumanalytics.com.au
+61 407 260 481

KPV

CAS Number : 67727-97-3

PubChem CID : 125672

Liquid Chromatography Mass Spectrometry (LC-MS) Identity Analysis

Identity confirmation with SIM


Analysis date : 12/09/2026

Monitored Ion Channels (SIM):

Monitored (m/z):	Detected (m/z):
343	343.25
685	685.20
761	761.35

Detection Assignment: KPV

Collected Mass Spectrum

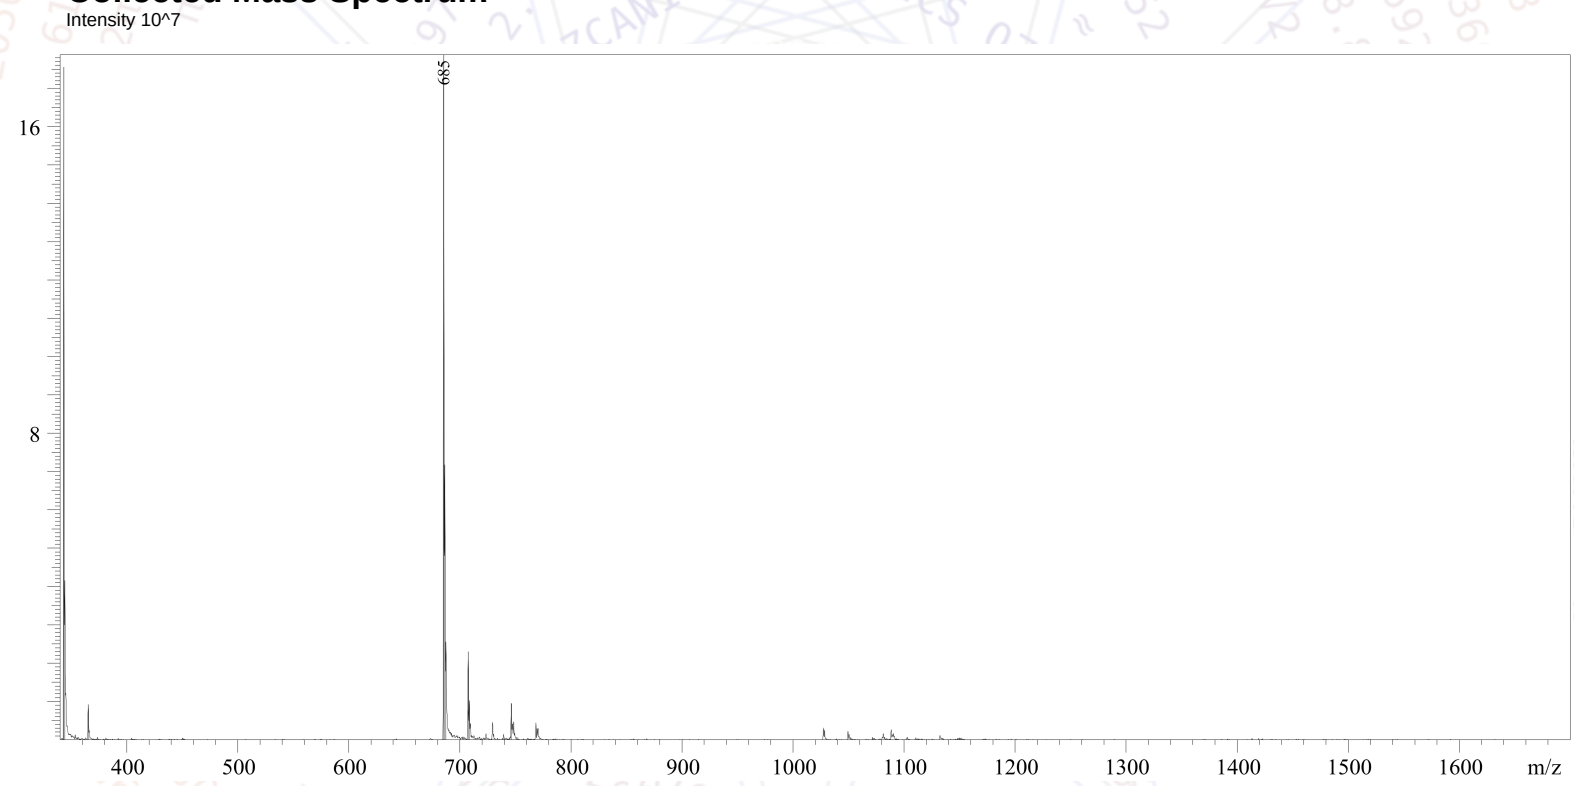

Note : Monoisotopic m/z values are not easily seen in full spectrum view for larger molecules and peptides.

The recorded fragmentation pattern may differ between systems, and vary based on method.

Analysis by Ibrahim A. Ozcan,
Lead Chemist Ozcanium Analytics
Signature

Report Compiled by Zein S. Sabini
14/09/2026

© Copyright 2026 by Ozcanium Analytics. All rights reserved.

Ozcanium Analytics
ABN: 14 754 514 569
Ozcaniumanalytics.com.au
+61 407 260 481

BPC-157

CAS Number : 137525-51-0 PubChem CID : 9941957

Liquid Chromatography Mass Spectrometry (LC-MS) Identity Analysis


Identity confirmation with SIM **Analysis date** : 12/09/2026

Monitored Ion Channels (SIM):

Monitored (m/z):	Detected (m/z):
711	710.85
947	947.25
1419	1419.10

Detection Assignment: BPC-157

Collected Mass Spectrum

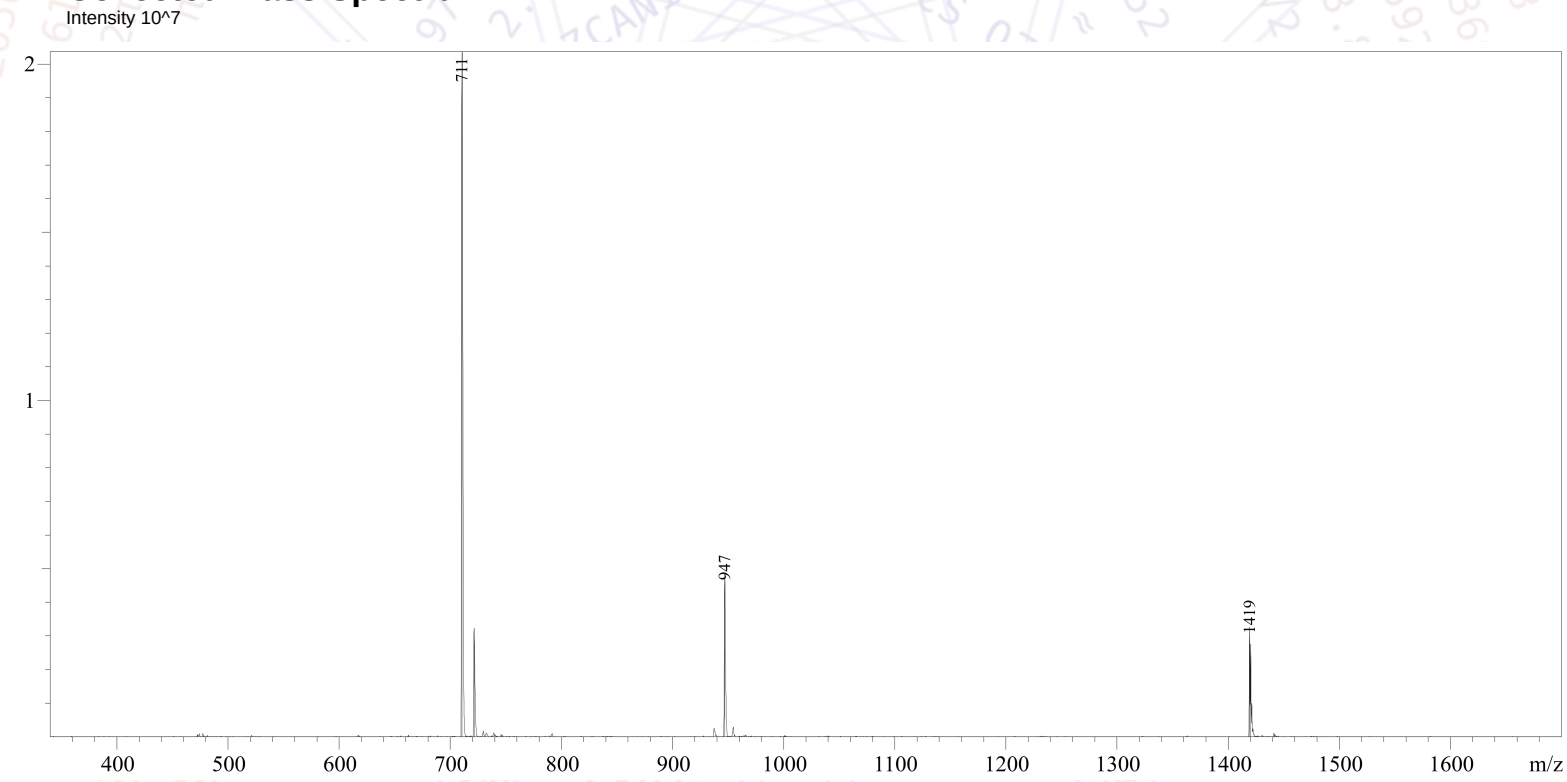

Note : Monoisotopic m/z values are not easily seen in full spectrum view for larger molecules and peptides.

The recorded fragmentation pattern may differ between systems, and vary based on method.

Analysis by Ibrahim A. Ozcan,
Lead Chemist Ozcanium Analytics
Signature

Report Compiled by Zein S. Sabini
14/09/2026

© Copyright 2026 by Ozcanium Analytics. All rights reserved.

Ozcanium Analytics
ABN: 14 754 514 569
Ozcaniumanalytics.com.au
+61 407 260 481

TB-500

CAS Number : 885340-08-9 PubChem CID : 16132341

Liquid Chromatography Mass Spectrometry (LC-MS) Identity Analysis


Identity confirmation with SIM **Analysis date** : 12/09/2026

Monitored Ion Channels (SIM):

Monitored (m/z):	Detected (m/z):
828	828.20
993	993.10
1241	1241.35

Detection Assignment: TB-500

Collected Mass Spectrum

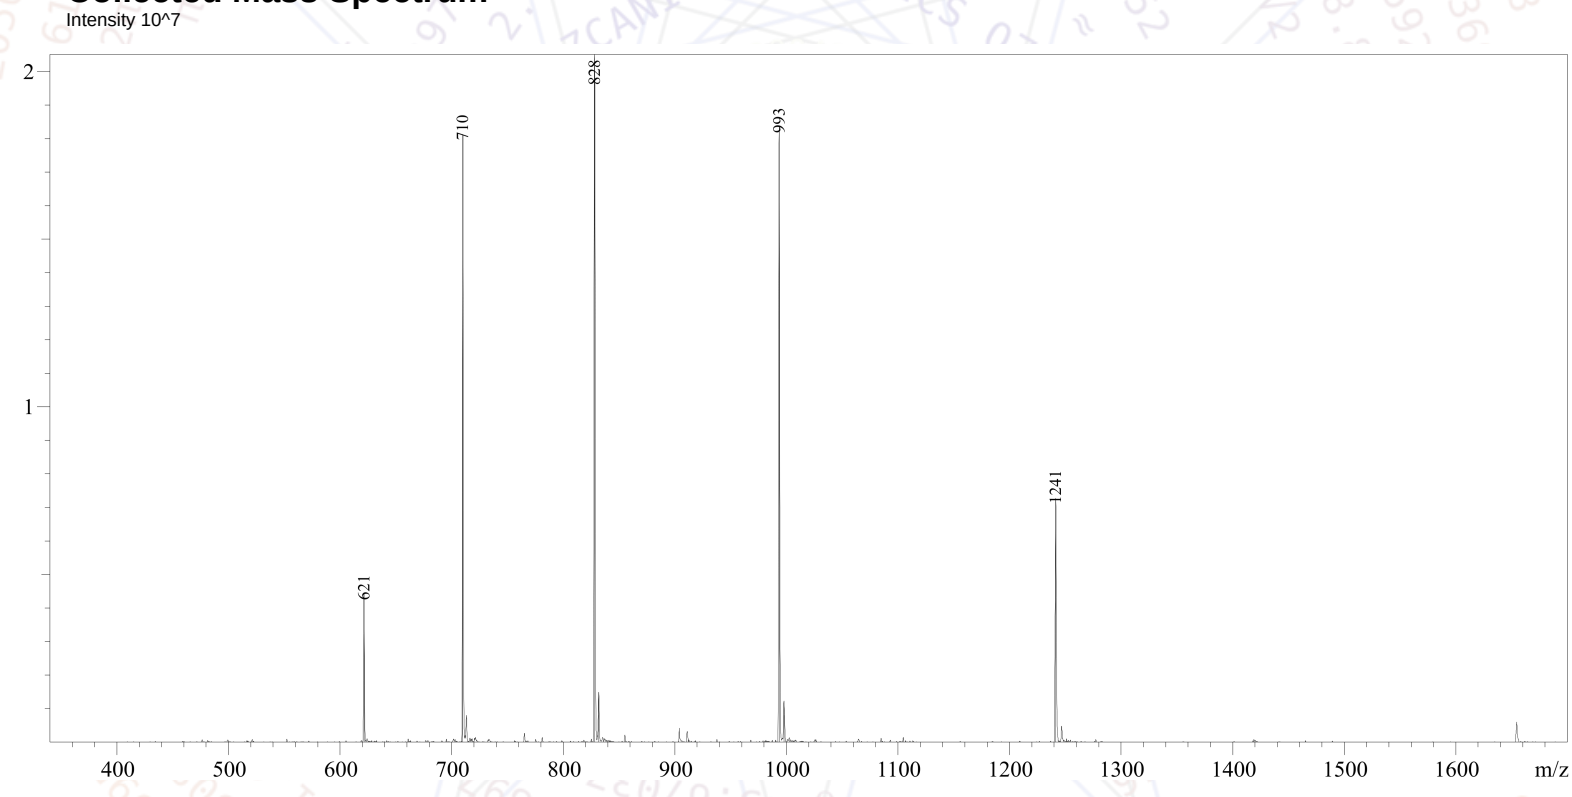

Note : Monoisotopic m/z values are not easily seen in full spectrum view for larger molecules and peptides.

The recorded fragmentation pattern may differ between systems, and vary based on method.

Analysis by Ibrahim A. Ozcan,
Lead Chemist Ozcanium Analytics
Signature

Report Compiled by Zein S. Sabini
14/09/2026

© Copyright 2026 by Ozcanium Analytics. All rights reserved.